

March 12, 2007



Instrumentation

Manufacturer

BERGOZ Instrumentation
01630 Saint Genis Pouilly, France
Fax: +33-450.426.642 Tel.: +33-450.426.643
sales@bergoz.com

Bergoz CT performance report



Distributors

U.S.A. : GMW Associates
955 Industrial Road
San Carlos, CA 94070, U.S.A.
Fax: (650) 802-8298 Tel.: (650) 802-8292
sales@gmw.com


Japan : REPIC Corporation
28-3, Kita Otsuka 1-Chome
Toshima-ku, Tokyo 170-0004, Japan
Fax: 03-3918-5712 Tel.: 03-3918-5326
sales@repic.co.jp

By Christophe Defrance

Test bench

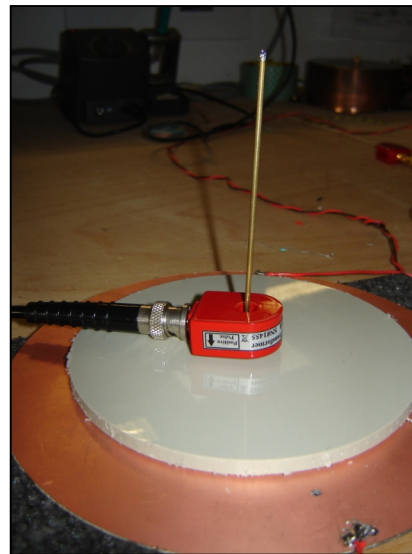
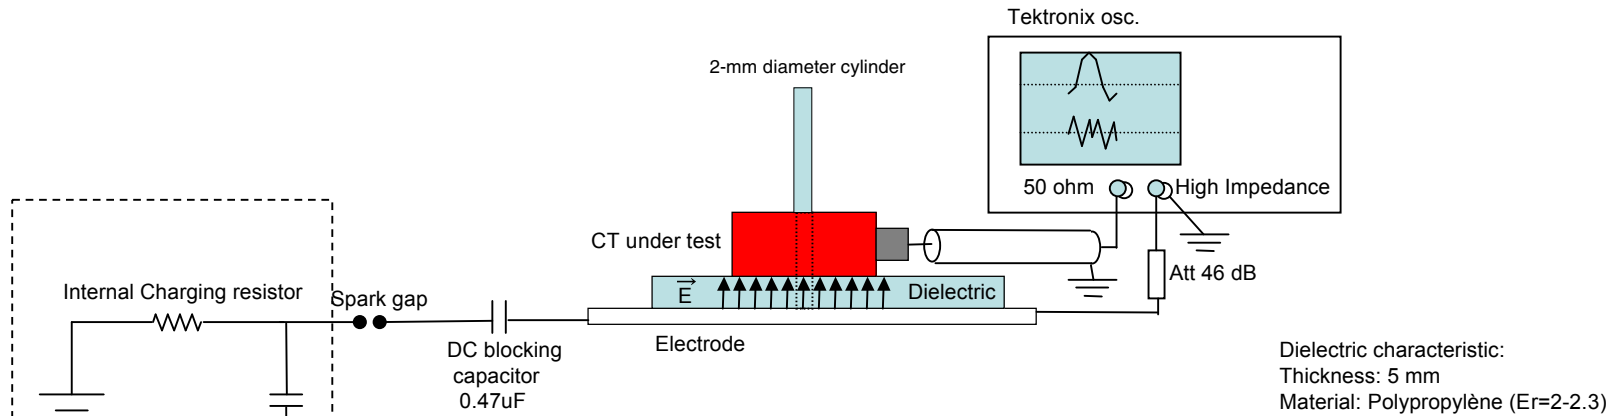


Flat electrode with cylinder through the CT


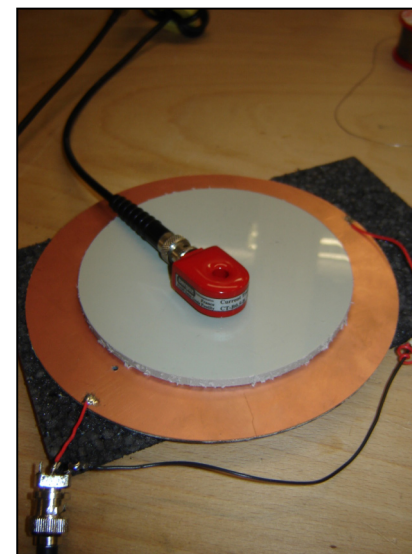


Flat electrode only

Measurements with flat electrode:

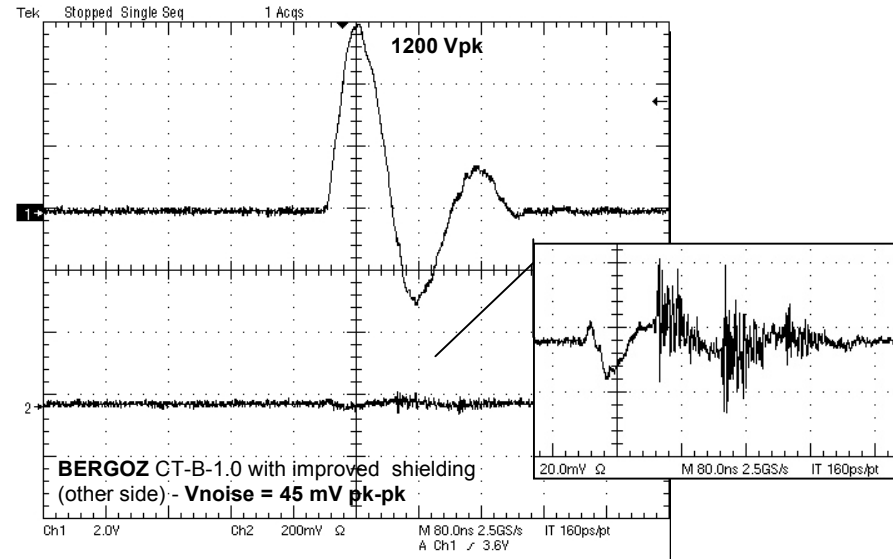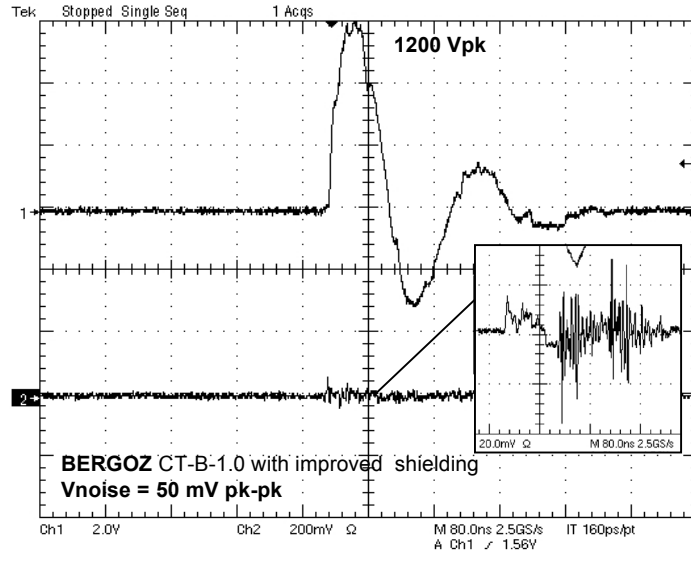

Measurements with flat electrode extended with a 2-mm diameter cylinder through the CT:

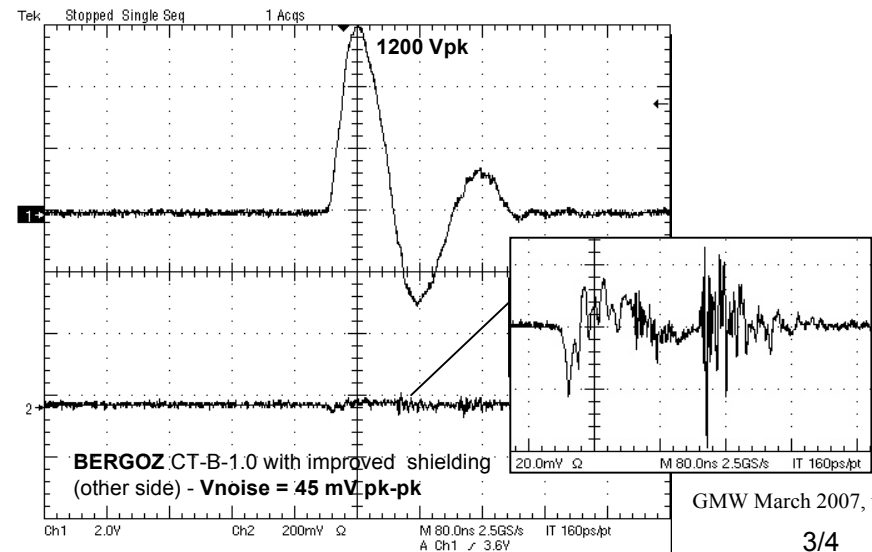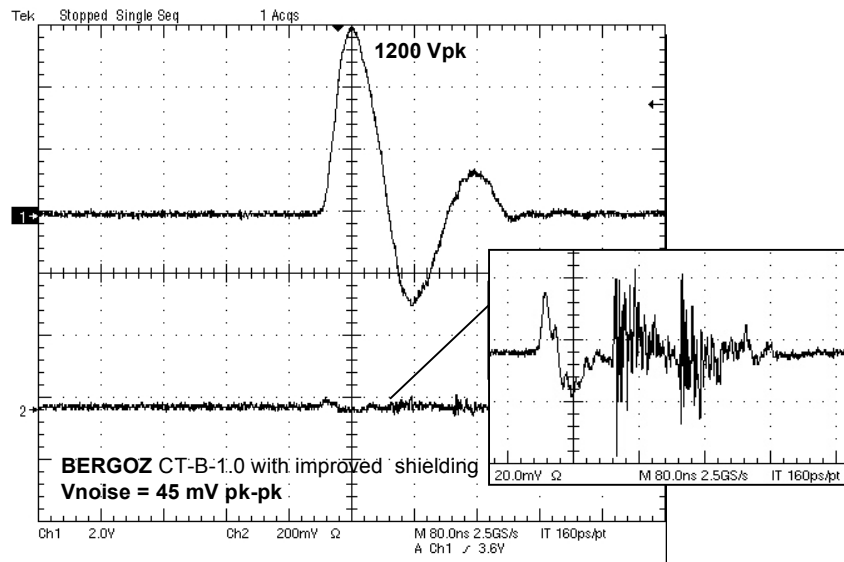

Bergoz CT amplitude & phase vs. frequency



Instrumentation

